



Instructions for use of NovoSeven® RT with pre-filled syringe

Overview – NovoSeven® RT with pre-filled syringe

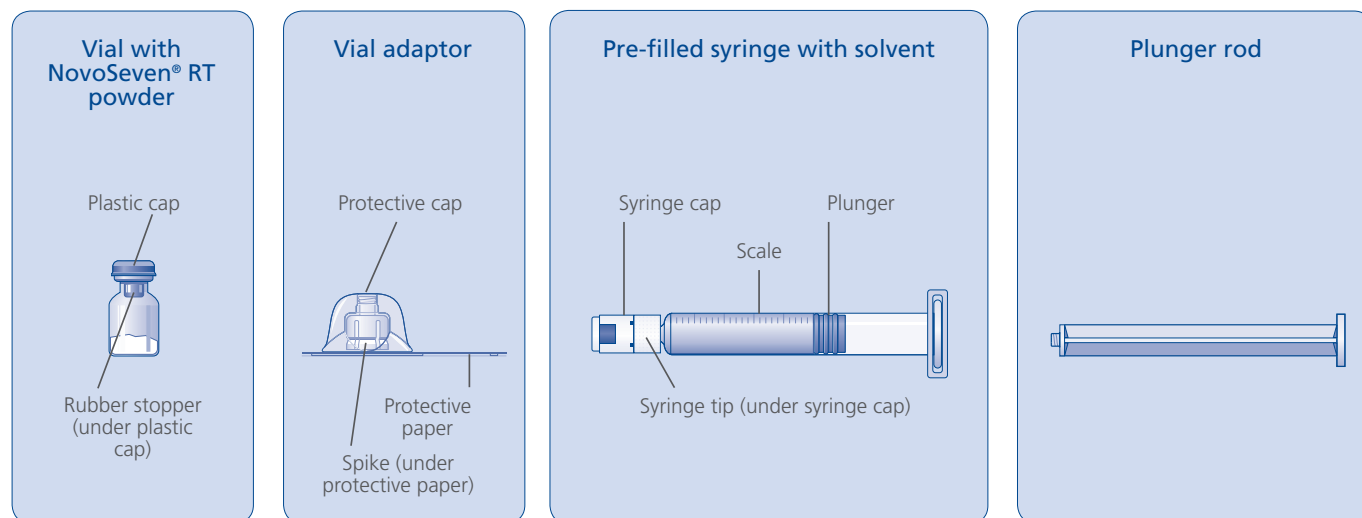


Prepare the treatment

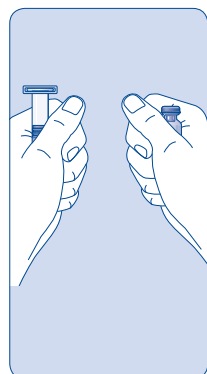

Check the expiry date, name and dose of each NovoSeven® RT package.

① Wash your hands before opening the carton.

If cold, warm the vial and pre-filled syringe in your hands (not above 37°C).

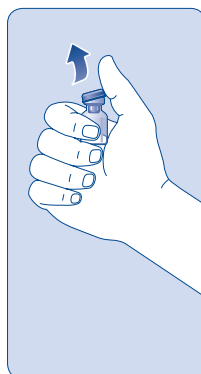


Remove the plastic cap from the vial.

Clean the rubber stopper with an alcohol swab and allow to dry.


STEP
1

Attach the vial adaptor

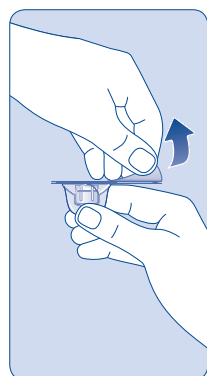

Remove the protective paper to open the vial adaptor protective cap.

① Do not touch the vial adaptor as it is sterile.

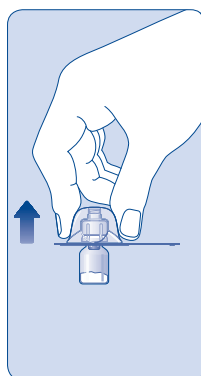

Turn the protective cap over, and snap the vial adaptor onto the vial.


Lightly squeeze the cap to remove it.

① Once attached, do not remove the vial adaptor from the vial.

STEP
2


Instructions for use of NovoSeven® RT with pre-filled syringe (cont.)

Attach the syringe and plunger rod

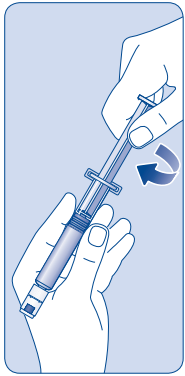


Insert the plunger rod into the syringe.

Turn it clockwise until tight.



Remove the syringe cap from the pre-filled syringe by bending it down until the perforation breaks.

ⓘ Do not touch or remove the white syringe tip under the syringe cap.




Screw the pre-filled syringe clockwise and securely onto the vial adaptor.

STEP
3

Mix the powder with the solvent



Hold at an angle and push the plunger rod to inject all the solvent into the vial.

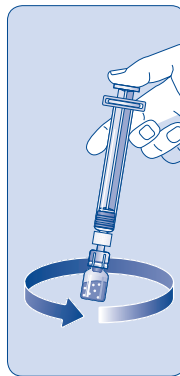


Keep the plunger rod pressed down and swirl the vial gently until all the powder is dissolved.

ⓘ Do not shake the vial, as this will cause foaming.

ⓘ Discard the mixed solution if there are visible particles or if it is not clear and colourless.

STEP
4a

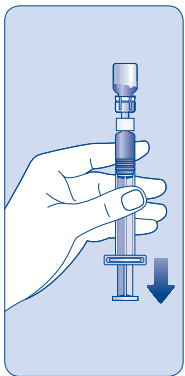


Turn the syringe upside down.


Release the plunger rod to let the solution enter the syringe.

Pull the plunger rod slightly downwards to draw the solution into the syringe.

While holding the vial upside down, tap the syringe gently to let any air bubbles rise to the top.



Push the plunger rod slowly until all trapped air is gone.



Disconnect the syringe by unscrewing the vial adaptor.

STEP
4b

NovoSeven® RT is now ready for use.

Inject intravenously over 2 to 5 minutes.

- ⓘ Use the mixed NovoSeven® RT at once.**
- ⓘ Discard all waste materials safely (including any unused NovoSeven® RT) into an appropriate container.**
- ⓘ Do not disassemble before disposal.**
- ⓘ Do not reuse.**

In case you need to mix several vials at one time for infusion in a large single syringe, please obtain advice on the correct procedure from a healthcare professional at the haemophilia treatment centre.

Further information: Novo Nordisk Customer Care Centre (Australia) 1800 668 626.

Novo Nordisk Pharmaceuticals Pty Ltd ABN 40 002 879 996
Level 3, 21 Solent Circuit, Baulkham Hills NSW 2153
www.novonordisk.com.au

® Registered trademarks of Novo Nordisk A/S.
© 2013 Novo Nordisk Pharmaceuticals Pty Ltd.

N7AUNZ465 | FD13832 | Prepared: Nov 2013

