## RCH Devices

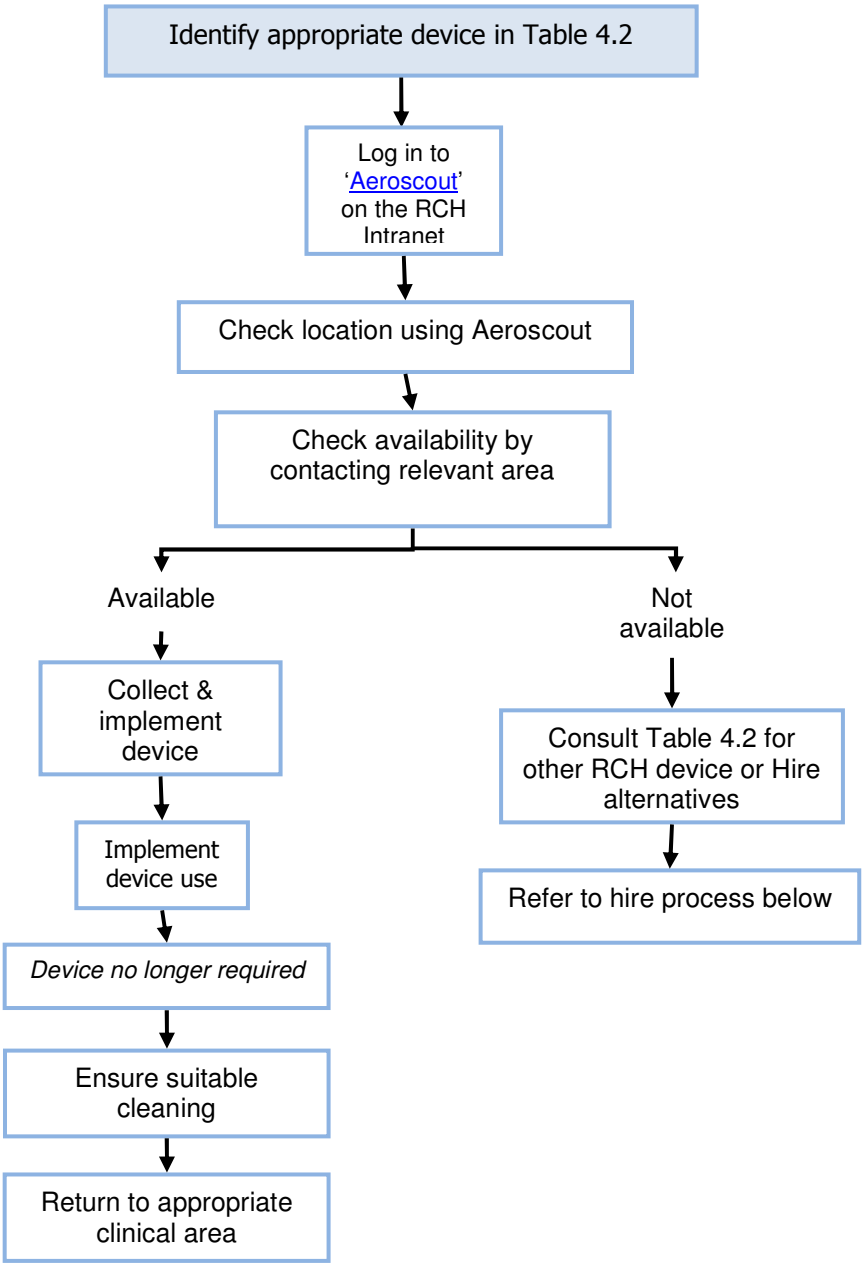
Identify appropriate device in Table 4.2
Log in to 'Aeroscout' on the RCH Intranet
Check location using Aeroscout
Check availability by contacting relevant area
Available
Not available
Collect & implement device
Implement device use
Device no longer required
Ensure suitable cleaning
Return to appropriate clinical area
Consult Table 4.2 for other RCH device or Hire alternatives
Refer to hire process below